

GE Healthcare

Thermo Sequenase Fluorescent Labelled Primer Cycle Sequencing Kit with 7-Deaza-dGTP

Product Booklet

Codes: RPN2438
RPN2538



Page finder

1. Legal	3
2. Handling	4
2.1. Safety warnings and precautions	4
2.2. Storage	5
3. Components of the system	6
4. Description	7
4.1. Quality control	7
4.2. Storage	7
5. Additional reagents and materials required	8
6. Thermo Sequenase fluorescent labelled primer cycle sequencing with 7-deaza-dGTP	9
6.1. Preparation of template DNA	9
6.2. Thermo Sequenase cycle sequencing with 7-deaza-dGTP and fluorescent 4 dye primer labelling	9
6.3. Thermo Sequenase cycle sequencing with 7-deaza-dGTP and fluorescent 1 dye primer labelling	16
7. Additional information	22
7.1. Sequencing the products of a polymerase chain reaction	22
7.2. Supplementary protocols	23
8. Troubleshooting guide	25
9. Background and references	28
9.1. Thermo Sequenase DNA polymerase	28
9.2. Cycle sequencing	28
10. Related products available from GE Healthcare	30
10.1. Sequencing reagents	30
10.2. DYEnamic ET primers	30
11. Thermo Sequenase fluorescent labelled primer cycle sequencing kits with 7-deaza-dGTP	31

1. Legal

GE and GE monogram are trademarks of General Electric Company. Thermo Sequenase, Sequenase and DYEnamic are trademarks of GE Healthcare companies.

This product is sold under licensing arrangements with Roche Molecular Systems, F Hoffmann-La Roche Ltd and the Perkin-Elmer Corporation. Purchase of this product is accompanied by a limited license to use it in the Polymerase Chain Reaction (PCR) process for research in conjunction with a thermal cycler whose use in the automated performance of the PCR process is covered by the up-front license fee, either by payment to Perkin-Elmer or as purchased, i.e. an authorized thermal cycler.

Tween is a trademark of ICI Americas Inc

Nonidet and Nescofilm are trademarks of Shell International Petroleum Co Ltd

Sigma is a trademark of Sigma Chemical Co

Parafilm is a trademark of American National Can

7-deaza-dGTP is licensed from Boehringer Mannheim GmbH

© 2006 General Electric Company – All rights reserved.

GE Healthcare reserves the right, subject to any regulatory approval, to make changes in specifications and features shown herein, or discontinue the product described at any time without notice or obligation.

Contact your GE Healthcare representative for the most current information and a copy of the terms and conditions.

<http://www.gehealthcare.com/lifesciences>

2. Handling

2.1. Safety warnings and precautions

Warning: For research use

only. Not recommended or intended for diagnosis of disease in humans or animals. Do not use internally or externally in humans or animals.

All chemicals should be considered as potentially hazardous. We therefore recommend that this product is handled only by those persons who have been trained in laboratory techniques and that it is used in accordance with the principles of good laboratory practice. Wear suitable protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken to avoid contact with skin or eyes. In the case of contact with skin or eyes, wash immediately with water. See material safety data sheet(s) and/or safety statements for specific advice).

Note that the protocol requires the use of acrylamide and NN'-methylenebisacrylamide.

Warning: Acrylamide and NN'-methylenebisacrylamide are toxic and classified as carcinogens. Please follow the manufacturers safety data sheet relating to the safe handling and use of these materials.

Note that the protocol requires the use of NNN'N'-tetramethylethylene diamine (TEMED) and ammonium peroxydisulphate (ammonium persulphate, AMPS).

Warning: NNN'N'-tetramethylethylene diamine and ammonium peroxydisulphate are classified as harmful and flammable. Please follow the manufacturers safety data sheets relating to the safe handling and use of these materials.

Note that the protocol requires the use of ethanol.

Warning: Ethanol is classified as flammable. Please follow the manufacturers safety data sheet relating to the safe handling and use of this material.

2.2. Storage

Store at -15°C to -30°C.

3. Components of the system

Each pack contains the following components:

Component	Contents	Cap colour
A reagent	Tris-HCl (pH 9.5), magnesium chloride, Tween™20, Nonidet™ P-40, 2-mercaptoethanol, dATP, dCTP, 7-deaza-dGTP, dTTP, ddATP, thermostable pyrophosphatase and Thermo Sequenase DNA polymerase	green
C reagent	Tris-HCl (pH 9.5), magnesium chloride, Tween 20, Nonidet P-40, 2-mercaptoethanol, dATP, dCTP, 7-deaza-dGTP, dTTP, ddCTP, thermostable pyrophosphatase and Thermo Sequenase DNA polymerase	blue
G reagent	Tris-HCl (pH 9.5), magnesium chloride, Tween 20, Nonidet P-40, 2-mercaptoethanol, dATP, dCTP, 7-deaza-dGTP, dTTP, ddGTP, thermostable pyrophosphatase and Thermo Sequenase DNA polymerase	yellow
T reagent	Tris-HCl (pH 9.5), magnesium chloride, Tween 20, Nonidet P-40, 2-mercaptoethanol, dATP, dCTP, 7-deaza-dGTP, dTTP, ddTTP, thermostable pyrophosphatase and Thermo Sequenase DNA polymerase	red
Formamide loading dye	Formamide, EDTA and fuchsin	clear

4. Description

Thermo Sequenase™ fluorescent labelled primer cycle sequencing kits with 7-deaza-dGTP* are recommended for fluorescent dye primer sequencing of single stranded or double stranded DNA templates.

4.1. Quality control

The Thermo Sequenase fluorescent labelled primer cycle sequencing kit with 7-deaza-dGTP is tested in fluorescent sequencing as follows:

DNA templates

XL-1 Blue/NZY propagated M13mp8 ssDNA.

TOP 10F/TSB propagated pBluescript miniprep dsDNA, prepared by a modification of the alkaline lysis method.

M13mp8 ssDNA from CsCl template preparation.

pUC18 dsDNA from CsCl template preparation.

Assay method

ABI 373 34 cm well-to-read and 4 dye-primer cycle sequencing with Thermo Sequenase DNA polymerase.

Quality

98.5% accurate from 20 bases beyond the 3'-end of the primer to 500 bases beyond the 3'-end of the primer.

4.2. Storage

The components in this kit may be stored at either 2-8°C or -15°C to -30°C with no difference in stability over 3 months. For longer term storage, we recommend -15°C to -30°C.

* See legal section page 3

5. Additional reagents and materials required

Reagents and materials that may be required but which are not supplied with the kit are detailed below. Many of these items are available from GE Healthcare. Please refer to the section on **related products available from GE Healthcare** on page 30 of this booklet.

Fluorescent dye labelled primers	for fluorescent sequencing. A range of dye labelled primers can be obtained for use with commercially available sequencing instruments.
Acrylamide gel electrophoresis materials	for separation of the sequencing reaction products. See the supplementary protocols section on page 23 of this booklet.
Light mineral oil	for overlaying the sequencing reactions. Use Sigma™ light mineral oil (catalogue code M-3516).

6. Thermo Sequenase fluorescent labelled primer cycle sequencing with 7-deaza-dGTP

6.1. Preparation of template DNA

High quality template DNA is essential to obtain the best results from the Thermo Sequenase fluorescent labelled primer cycle sequencing kit with 7-deaza-dGTP. Protocols and reagent kits are available from GE Healthcare for the preparation of M13 and plasmid sequencing templates.

6.2. Thermo Sequenase cycle sequencing with 7-deaza-dGTP and fluorescent 4 dye primer labelling

The reagents in the Thermo Sequenase fluorescent labelled primer cycle sequencing kit with 7-deaza-dGTP are suitable for use with fluorescently labelled primers such as those used with the Applied Biosystems 373 and 377 Fluorescent Sequencers.

1. Remove the following components from the kit and allow to thaw (if stored frozen): A reagent (green cap), C reagent (blue cap), G reagent (yellow cap), T reagent (red cap) and formamide loading dye (for fluorescent samples) (clear cap). Store on ice until required. All of the tubes should be well mixed before use by briefly vortexing the tube.
2. Prepare any other materials that may be required. The following quantities of template are recommended: 0.5–2 µg of single stranded DNA or 0.5–5 µg of double stranded DNA. The DNA should be in a total volume of at least 30 µl. If the template is the product of a polymerase chain reaction (PCR)*, please refer to the section on sequencing the products of PCR on page 22 of this booklet.

*See Legal chapter on page 3.

3. Label four tubes or microplate wells as follows: A reaction, C reaction, G reaction and T reaction. Reactions should be prepared as shown below:

A and C reactions

	For each sample:
Primer (JOE for A terminations, FAM for C terminations)	1 μ l
Template DNA	5 μ l
A or C reagent	2 μ l

Reagents and primers may be conveniently premixed before addition to the template DNA. The following table gives the volumes of primers and reagents needed for some commonly used numbers of samples.

Number of samples	Primer	Reagent	Total volume
	JOE FAM	A C	
4	4 μ l	8 μ l	12 μ l
8	8 μ l	16 μ l	24 μ l
12	12 μ l	24 μ l	36 μ l
16	16 μ l	32 μ l	48 μ l
24	24 μ l	48 μ l	72 μ l

Mix thoroughly after the addition of each reagent by pipetting up and down two or three times. The premixes can be freshly prepared for each set of sequencing reactions or they can be prepared in bulk and stored at 2–8°C. Premixes should be kept on ice until used.

G and T reactions

	For each sample:
Primer (TAMRA for G terminations, ROX for T terminations)	2 μ l
Template DNA	10 μ l
G or T reagent	4 μ l

Again, reagents and primers may be conveniently premixed before addition to the template DNA. The following table gives the volumes of primers and reagents needed for some commonly used numbers of samples.

Number of samples	Primer	Reagent	Total volume
	TAMRA ROX	G T	
4	8 μ l	16 μ l	24 μ l
8	16 μ l	32 μ l	48 μ l
12	24 μ l	48 μ l	72 μ l
16	32 μ l	64 μ l	96 μ l
24	48 μ l	96 μ l	144 μ l

Mix thoroughly after the addition of each reagent by pipetting up and down two or three times. Again, the premixes can be freshly prepared for each set of sequencing reactions or they can be prepared in bulk and stored at 2–8°C. Premixes should be kept on ice until used.

- When all of the reactions have been prepared; overlay with light mineral oil, or add a wax barrier pellet, or cap the tube with an evaporation-preventing lid as appropriate for your thermocycler. We recommend an overlay with 50 μ l of light mineral oil for reactions in standard 96 well microplates and 1.5 ml microcentrifuge tubes.
- Thermocycle the reactions. The exact thermocycling conditions will depend upon the primer set used, the degree of amplification required, the type of template (ssDNA or dsDNA) and the amount of template. The best thermocycling conditions can only be found by experiment. Some recommended starting conditions for the optimisation of the thermocycling conditions are given below. Note that the conditions given are only guidelines in order to start this optimisation process.

Primer set	Template	Amount	Annealing	Denaturation	Number of cycles
DYEnamic ET primers	plasmid dsDNA	>1 µg	50°C, 30 sec	95°C, 30 sec	7-8*
-40 M13 forward	plasmid dsDNA	<1 µg	50°C, 30 sec	95°C, 30 sec	10
US 79339	M13 ssDNA	>1 µg	50°C, 30 sec	95°C, 30 sec	3-5
(500 templates)	M13 ssDNA	<1 µg	50°C, 30 sec	95°C, 30 sec	5
-28 M13 reverse					
US 79357					
(500 templates)					
ABI T7	plasmid dsDNA	>1 µg	50°C, 30 sec	95°C, 30 sec	25
(#401127)	plasmid dsDNA	<1 µg	50°C, 30 sec	95°C, 30 sec	30
	M13 ssDNA	>1 µg	50°C, 30 sec	95°C, 30 sec	20
	M13 ssDNA	<1 µg	50°C, 30 sec	95°C, 30 sec	25
ABI T3	plasmid dsDNA	>1 µg	55°C, 30 sec	95°C, 30 sec	20
(#401128)	plasmid dsDNA	<1 µg	55°C, 30 sec	95°C, 30 sec	25
	M13 ssDNA	>1 µg	55°C, 30 sec	95°C, 30 sec	15
	M13 ssDNA	<1 µg	55°C, 30 sec	95°C, 30 sec	20
ABI SP6	plasmid dsDNA	>1 µg	55°C, 30 sec	95°C, 30 sec	20
(#401129)	plasmid dsDNA	<1 µg	55°C, 30 sec	95°C, 30 sec	25
	M13 ssDNA	>1 µg	55°C, 30 sec	95°C, 30 sec	15
	M13 ssDNA	<1 µg	55°C, 30 sec	95°C, 30 sec	20

*See Dyanamic™ ET primer protocol book for detailed reaction conditions


For very GC-rich samples, we recommend a denaturation temperature of 98°C.

In addition, a pre-denaturation for 5 minutes at 95°C may be beneficial for plasmid cycle sequencing.


For full details of related products see pages 30–31.

6. After the thermocycling has been completed, the A, C, G and T reactions should be pooled together. If an oil overlay has been used in order to prevent evaporation during the thermocycling, it is imperative that traces of oil are removed before ethanol precipitation is carried out. Residual oil droplets actually sink in ethanol and are immediately centrifuged to the bottom of the tube. The sequencing reaction may therefore be centrifuged on to this residual oil rather than the plastic surface of the tube. Removal of the ethanol-containing supernatant after centrifugation can easily result in loss of most or all of the sequenced DNA. We find the following technique for removal of residual oil both simple and completely effective.

Pool the sequencing reactions together using a P200 tip. Try to minimise the amount of oil taken but be sure to collect all of the sequencing reactions. Set up a 'slope' of Nescofilm™ or Parafilm™ as illustrated below. Pipette the pooled sequencing reactions and residual oil on to the top of the slope as shown:

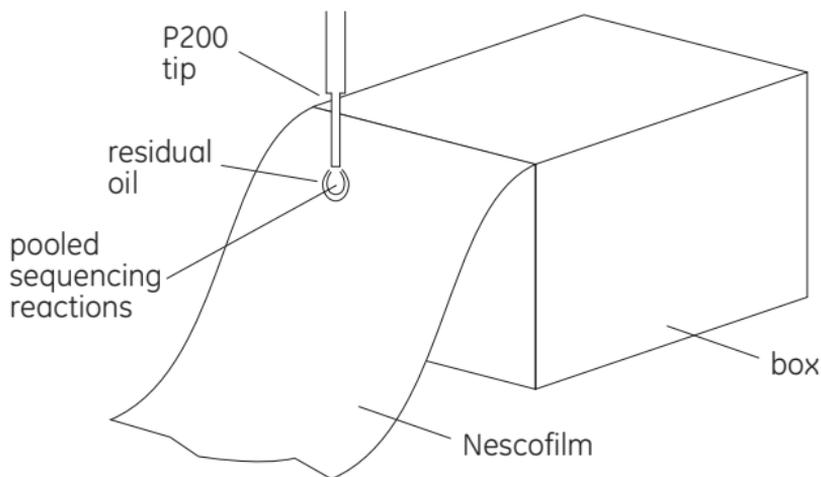

The pooled sequencing reactions will run down the slope, leaving a 'trail' of residual oil behind on the Nescofilm or Parafilm.

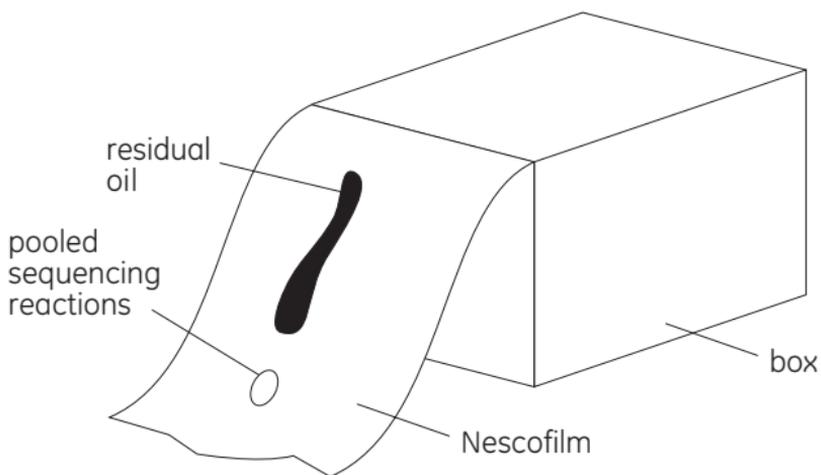

Use a **fresh** P200 tip to transfer the pooled sequencing reactions (now free of any residual oil) for ethanol precipitation.

7. When residual oil has been removed, the pooled sequencing reactions can be ethanol precipitated. We recommend the use of a hinged 1.5 ml microcentrifuge tube and the following protocol:


Add ~1/10th volume 3 M NaOAc (pH 5.2) (5 μ l)

Add 2.5 volumes of ethanol and mix well (132 μ l)

Leave for 5 minutes at room temperature.

Spin for 10 minutes in a microcentrifuge with the hinge of the tube facing **outwards**.

Remove tube and use a vacuum aspirator plus a fresh P200 tip to remove the supernatant. Place the P200 tip **opposite** the hinge for supernatant aspiration as shown below:

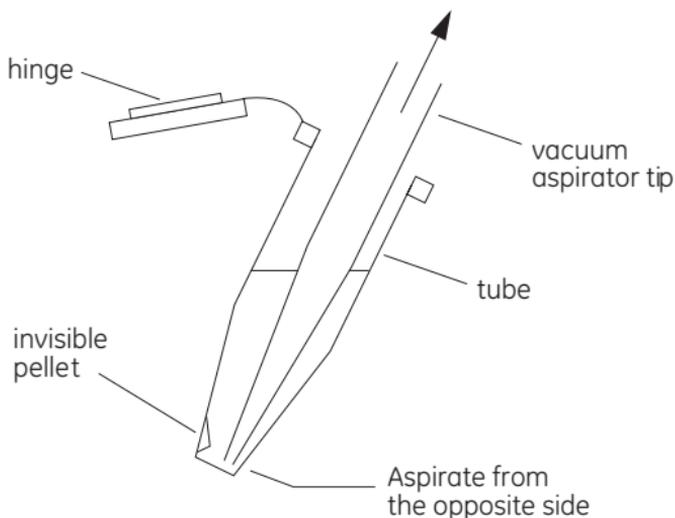

Gently add 500 μ l of 80% ethanol with a P1000 tip.

Use a vacuum aspirator plus a fresh P200 tip to remove the supernatant. There is no need to vortex the tube and re-spin (this only increases the chances of detaching the pellet from the tube wall). Again, place the P200 tip **opposite** the hinge for supernatant aspiration.

Add 2–5 μ l of formamide loading dye (for fluorescent samples) and vortex well or pipette up and down to resuspend. The exact volume of formamide loading dye (for fluorescent samples) used for resuspension will depend on the type of comb used for loading the sequencer.

8. Load the samples on the fluorescent sequencer. **Do not denature the samples.** Signal intensity is not affected. Denaturation of sequences containing 7-deaza-dGTP dissolved in formamide can lead to degradation and subsequent poor quality results.

6.3. Thermo Sequenase cycle sequencing with 7-deaza-dGTP and fluorescent 1 dye primer labelling

1. Remove the following components from the kit and allow to thaw (if stored frozen): A reagent (green cap), C reagent (blue cap), G reagent (yellow cap), T reagent (red cap) and formamide loading dye (for fluorescent samples) (clear cap). Store on ice until required. All of the tubes should be well mixed before use by briefly vortexing the tube.
2. Prepare any other materials that may be required. The following quantities of template are recommended: 0.5–2 μg of single stranded DNA or 0.5–5 μg of double stranded DNA. The DNA should be in a total volume of at least 20 μl . If the template is a PCR product please refer to the section on sequencing the products of a polymerase chain reaction on page 22 of this booklet.
3. Label four tubes or microplate wells as follows: A reaction, C reaction, G reaction and T reaction. Reactions should be prepared as follows:

	For each sample:
Fluorescent primer (1–2 pmol/ μl)	1 μl
Template DNA	5 μl
A, C, G or T reagent	2 μl

Reagents and primers may be conveniently premixed before addition to the template DNA. The following table gives the volumes of primers and reagents needed for some commonly used numbers of samples.

Number of samples	Primer	Reagent A, C, G or T	Total volume
4	4 μ l	8 μ l	12 μ l
8	8 μ l	16 μ l	24 μ l
12	12 μ l	24 μ l	36 μ l
16	16 μ l	32 μ l	48 μ l
24	24 μ l	48 μ l	72 μ l

Mix thoroughly after the addition of each reagent by pipetting up and down two or three times. The premixes can be freshly prepared for each set of sequencing reactions or they can be prepared in bulk and stored at 2–8°C. Premixes should be kept on ice until used.

- When all of the reactions have been prepared; overlay with light mineral oil, or add a wax barrier pellet, or cap the tube with an evaporation-preventing lid as appropriate for your thermocycler. We recommend an overlay with 50 μ l of light mineral oil for reactions in standard 96 well microplates and 1.5 ml microcentrifuge tubes.
- Thermocycle the reactions. The exact thermocycling conditions will depend upon the primer set used, the degree of amplification required, the type of template (ssDNA or dsDNA) and the amount of template. The best thermocycling conditions can only be found by experiment. Some recommended starting conditions for the optimisation of the thermocycling conditions are given below. Note that the conditions given are only guidelines in order to start this optimisation process.


Primer set	Template	Amount	Annealing	Denaturation	Number of cycles
M13 universal	plasmid dsDNA	>1 µg	60°C, 30 sec	95°C, 30 sec	20
	plasmid dsDNA	<1 µg	60°C, 30 sec	95°C, 30 sec	25
	M13 ssDNA	>1 µg	60°C, 30 sec	95°C, 30 sec	15
	M13 ssDNA	<1 µg	60°C, 30 sec	95°C, 30 sec	20
M13 reverse	plasmid dsDNA	>1 µg	60°C, 30 sec	95°C, 30 sec	20
	plasmid dsDNA	<1 µg	60°C, 30 sec	95°C, 30 sec	25
	M13 ssDNA	>1 µg	60°C, 30 sec	95°C, 30 sec	15
	M13 ssDNA	<1 µg	60°C, 30 sec	95°C, 30 sec	20

For very GC-rich samples, we recommend a denaturation temperature of 98°C.


In addition, a pre-denaturation for 5 minutes at 95°C may be beneficial for plasmid cycle sequencing.

- After the thermocycling has been completed, the A, C, G and T reactions should each be ethanol precipitated. This results in the best possible gel resolution, however it is possible to omit this step and still obtain acceptable data quality. Users wishing to do this should follow the recommendations of the manufacturer of the particular fluorescent sequencer being used. If an oil overlay has been used in order to prevent evaporation during the thermocycling, it is imperative that traces of oil are removed before ethanol precipitation is carried out. Residual oil droplets actually sink in ethanol and are immediately centrifuged to the bottom of the tube. The sequencing reaction may therefore be centrifuged on to this residual oil rather than the plastic surface of the tube. Removal of the ethanol-containing supernatant after centrifugation can easily result in loss of most or all of the sequenced DNA. We find the following technique for removal of residual oil both simple and completely effective.

Recover each of the sequencing reactions using a fresh P200 tip for each one. Try to minimise the amount of oil taken but be sure to collect all of each sequencing reaction. Set up a 'slope' of Nescofilm or Parafilm as illustrated below. Pipette each of the sequencing reactions and residual oil on to the top of the slope as shown:

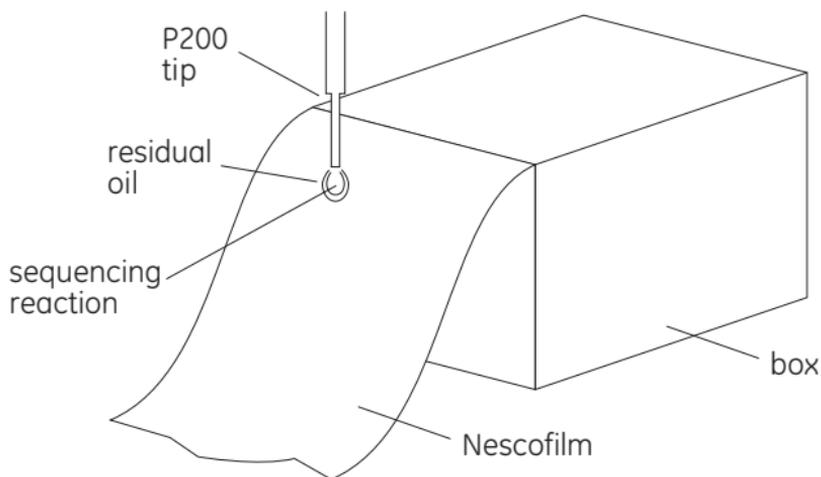

The sequencing reactions will run down the slope, leaving a 'trail' of residual oil behind on the Nescofilm or Parafilm.

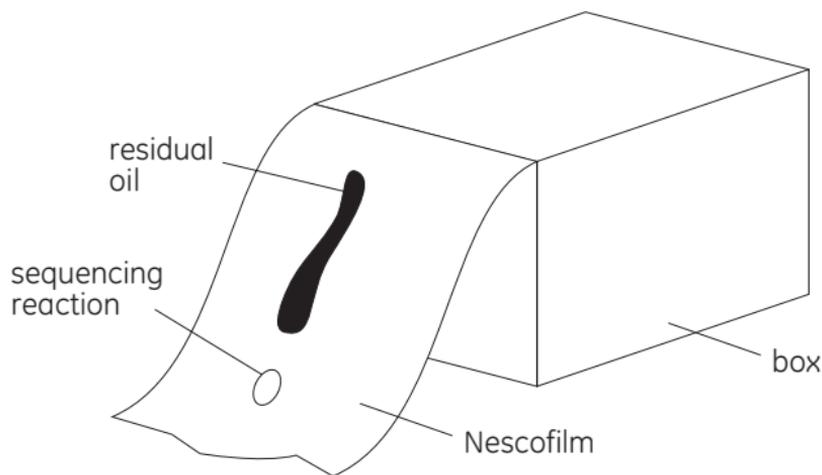

Use a fresh P200 tip to transfer the pooled sequencing reactions (now free of any residual oil) for ethanol precipitation.

- When residual oil has been removed, the sequencing reactions can be ethanol precipitated. We recommend the use of a hinged 1.5 ml microcentrifuge tube and the following protocol:


Add ~1/10th volume 3 M NaOAc (pH5.2) (1 μ l)

Add 2.5 volumes of ethanol and mix well (23 μ l)

Leave for 5 minutes at room temperature.

Spin for 10 minutes in a microcentrifuge with the hinge facing **outwards**.

Remove tube and use a vacuum aspirator plus a fresh P200 tip to remove the supernatant. Place the P200 tip **opposite** the hinge for supernatant aspiration as shown below:

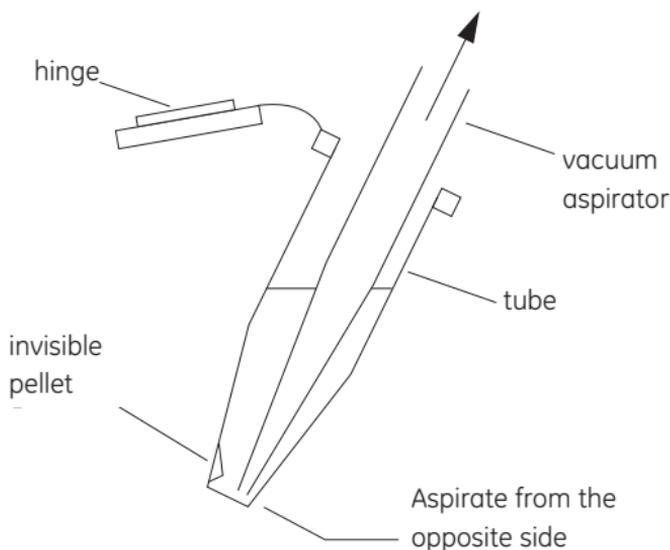

Gently add 500 μ l of 80% ethanol with a P1000 tip.

Use a vacuum aspirator plus a fresh P200 tip to remove the supernatant. There is no need to vortex the tube and re-spin (this

only increases the chances of detaching the pellet from the tube wall). Again, place the P200 tip **opposite** the hinge for supernatant aspiration.

Add 2–5 μl of formamide loading dye (for fluorescent samples) and vortex well or pipette up and down to resuspend. The exact volume of formamide loading dye (for fluorescent samples) used for resuspension will depend of the type of comb used for loading the sequencer.

8. Load the samples on the fluorescent sequencer. **Do not denature the samples.** Signal intensity is not affected. Denaturation of sequences containing 7-deaza-dGTP dissolved in formamide can lead to degradation and subsequent poor quality results.

7. Additional information

7.1. Sequencing the products of a polymerase chain reaction

DNA generated by the polymerase chain reaction (PCR)(4) may also be used as a template for sequencing. The pre-treatment of the PCR product with the GE Healthcare reagent pack for PCR product sequencing (US 70995) is recommended.

It is also possible to successfully sequence unpurified PCR products using a simple dilution protocol. The following section contains guidelines about how to use this approach.

- The dilution method relies on the PCR product being as homogeneous as possible. Care should be taken in the design of the PCR to ensure that truncated and misprimed fragments are minimised. PCR products should be analysed on an agarose gel to check the homogeneity of the product.
- In general, it is better to use a different primer for the sequencing reaction than was used for the PCR. We recommend that the 5'-end of the sequencing primer is positioned at least 20 bases from the 3'-end of the PCR primer.
- The dilution of the PCR product that will be required will vary according to the size and concentration. We recommend that a series is carried out to find the optimum dilution for each PCR product. In general, we have found that dilutions in the range 1:10 to 1:100 are suitable for most cases.
- If possible, sequence the PCR product with both forward and reverse sequencing primers.

7.2. Supplementary protocols

Preparation of a 6% acrylamide gel mix

The preparation of a high quality gel mix is important in obtaining the maximum amount of data from the separated sequencing reactions. This is particularly critical when using fluorescent detection.

Premixed acrylamide stocks are available from a number of manufacturers. These are usually supplied as preweighed powders containing a 19:1 acrylamide/bis-acrylamide mixture that can be used to make a 40% solution. Once the 40% solution has been prepared, it should be stored at 2–8°C in the dark. Acrylamide solutions should be stored for no longer than two weeks.

The 6% acrylamide gel mix is prepared as follows. The quantities below produce 500 ml of gel mix. This can be used for up to a week.

1. Weigh out 250 g of urea (electrophoresis grade).
2. Add 75 ml of 40% acrylamide stock solution.
3. Add 187.5 ml of deionised water.
4. Add 3–5 g of mixed bed resin.
5. The urea can be dissolved by gently heating the solution while stirring.

Be careful not to overheat the solution - a stream of water from a hot water tap on the outside of the beaker should be sufficient to dissolve the urea.

Warning: Never microwave solutions containing acrylamide.

6. Filter 50 ml of 10 × TBE through a 0.2 µm cellulose acetate filter. Filter the acrylamide solution through the same filter into the same container. Degas for 5 minutes.
7. Store the gel mix at 2–8°C in the dark.

The gel plates should be cleaned and assembled using standard procedures. For fluorescent sequencing, follow the recommendations from the manufacturer of the sequencer.

Immediately before pouring the gel add 1/1000 volume of NNN'N'-tetramethylethylene diamine (TEMED) and 1/200 volume of 10% ammonium persulphate (AMPS). For example, for 80 ml of gel mix, add 80 μ l of TEMED and 0.40 ml of AMPS. Solutions of AMPS should always be freshly prepared.

Mix well and pour the gel. Allow 1–2 hours for polymerisation before using the gel.

8. Troubleshooting

Sequencing chemistry problems

Problem	Possible cause	Action
1. Faint or no sequence on all samples	1. Insufficient template DNA	1. Check an aliquot of the template preparation on an agarose gel to assess the yield. Ensure that at least 0.5–2 µg ssDNA or 0.5–5 µg dsDNA was used for fluorescent sequencing.
	2. Missing reaction component	2. Check that all of the premixes were prepared correctly.
	3. Inactive enzyme	3. When stored under the recommended conditions Thermo Sequenase DNA polymerase should be stable for greater than 6 months. Check that the enzyme has been correctly stored and that the kit is within the stated expiry date.
	4. No priming	4. Check that the primer is suitable for the template to be sequenced.

Problem	Possible cause	Action
2. High background on sequence	1. Poor quality DNA preparation	1. Check the DNA preparation on an agarose gel.
	2. Plasmid propagated in an <i>endA1+</i> strain	2. Some common <i>endA1+</i> strains such as TG1 can produce plasmids which give a high background on sequencing.
	3. Secondary priming sites	3. Check the sequencing primer for homology to other sequences in the vector, particularly within the 8–10 bases at the 3'-end. If there is a problem with secondary binding, the background is usually seen as specific bands rather than generalised background. Try using a different primer.
3. Bands smeared	1. Poor quality gel materials	1. Follow the recommendations in the section on preparation of a 6% acrylamide gel mix on page 23 of this booklet.
	2. Samples denatured	2. Ensure that samples are not denatured before loading.

Problem	Possible cause	Action
4. Bands across all four tracks	1. Poor quality DNA	1. Check the DNA preparation on an agarose gel.
	2. Strong secondary structure	2. The enzyme may pause at sites of high secondary structure. If possible, try sequencing the other strand.
5. Very short length of read in fluorescent sequencing	1. Plasmid propagated in an <i>endA1+</i> strain	1. Some common <i>endA1+</i> strains such as TGI can produce plasmids which give a high background and short read length in fluorescent sequencing.

If problems persist, please contact GE Healthcare Technical Services for assistance. Please be prepared to give as much information as possible about the exact circumstances under which the problem occurred and always quote the batch number of any reagents that you have used.

9. Background and references

9.1. Thermo Sequenase DNA polymerase

Thermo Sequenase is a heat stable DNA polymerase producing even band intensities in DNA sequencing. GE Healthcare have used a recent discovery of Tabor and Richardson (1) to construct this exonuclease-free thermostable DNA polymerase. Like Sequenase™ T7 DNA polymerase, Thermo Sequenase generates uniform (and therefore easy to read) sequence band patterns. However, the thermostability of this enzyme also makes it suitable for cycle sequencing. Thermo Sequenase therefore combines accuracy comparable with Sequenase T7 DNA polymerase with the sensitivity of cycle sequencing.

9.2. Cycle sequencing

DNA sequencing relies on the synthesis of a new strand of DNA starting at a specific priming site and ending with the incorporation of a chain terminating nucleotide such as a dideoxynucleoside triphosphate (2).

In fluorescent dye-primer sequencing and radioactive primer sequencing, the label is incorporated on the 5'-end of the primer. The relative concentrations of dNTPs and ddNTPs are balanced so that, on average, at each position within the desired length of sequence, there is an equal chance of a ddNTP being incorporated.

When these fragments are separated on a suitable gel matrix, sequence information can be obtained. The inclusion of 7-deaza-dGTP in the nucleotide mixes of this kit effectively eliminates 'compression' artefacts during gel electrophoresis.

Cycle sequencing (3) uses repeated cycles of thermal denaturation, annealing and extension/termination to increase signal levels and therefore decrease the amount of template required. For each

cycle, the amount of product DNA will be equivalent to the amount of primed template. However, if a thermostable enzyme such as Thermo Sequenase DNA polymerase is used, many cycles can be performed without the need to add fresh enzyme.

For example, after ten cycles there could be up to ten times as much product as template (in practice, each cycle is not 100% efficient and the amplification is somewhat lower than this).

Cycle sequencing is therefore ideally suited for applications where the amount of template may be limiting or where the sensitivity of the detection system is not high. For these reasons, we recommend using the Thermo Sequenase fluorescent labelled primer cycle sequencing kit with 7-deaza-dGTP for fluorescent sequencing using dye labelled primers.

1. Tabor, S. and Richardson, C., *Proc. Natl. Acad. Sci. (USA)*.
2. Sanger, F., Niklen, S. and Coulson, A.R., *Proc. Natl. Acad. Sci. (USA)*, **74**, pp. 5463-5467, 1977.
3. Murray, V. *et al.*, *Nucleic Acids Research*, **17**, p.8889, 1989.
4. Saiki, R.K. *et al.*, *Science*, **230**, pp.1350-1354, 1985.

10. Related products available from GE Healthcare

10.1. Sequencing reagents

Product	Application	Pack size	Product number
Acrylamide, Ultrapure	Gel electrophoresis	1 kg	US 75820-1KG
		500 g	US 75820-500G
Boric acid	Electrophoresis buffer	1 kg	US 76324-1KG
DNA sequencing gel mix, 6%, Ultrapure	Supplied with TBE running buffer. Each bottle makes 125 ml of gel solution	5 bottles	US 72990-5BTL
DNA sequencing gel mix, 8%, Ultrapure	Supplied with TBE running buffer. Each bottle makes 125 ml of gel solution	5 bottles	US 70090-5BTL
N,N'-methylene-bis acrylamide, Ultrapure	Gel electrophoresis	1 kg	US 75821-1KG
		500 g	US 75821-500G
Urea, Ultrapure	Gel electrophoresis	1 kg	US 75826-1KG
		500 g	US 75826-500G

10.2. DYEnamic ET primers

DYEnamic ET primers for 4 dye labelled primer sequencing

Primer	Pack size	Product code
-40 M13 forward primer	100 templates (Start up kit)	US 79345
5'-GTTTTCCCAGTCACGACG-3'	500 templates	US 79339
	10 000 templates	US 79340
-28 M13 reverse primer		
5'-AGGAAACAGCTATGACCAT-3'	500 templates	US 79355
	10 000 templates	US 79357

11. Thermo Sequenase fluorescent labelled primer cycle sequencing kits with 7-deaza-dGTP

RPN 2438 Thermo Sequenase fluorescent labelled primer cycle sequencing kit with 7-deaza-dGTP

Sufficient for 100 templates

A reagent 1 tube

C reagent 1 tube

G reagent 1 tube

T reagent 1 tube

Formamide loading dye
(for fluorescent samples) 2 tubes

RPN 2538 Thermo Sequenase fluorescent labelled primer cycle sequencing kit with 7-deaza-dGTP

Sufficient for 500 templates

A reagent 5 tubes

C reagent 5 tubes

G reagent 5 tubes

T reagent 5 tubes

Formamide loading dye
(for fluorescent samples) 1 x 10 ml

GE Healthcare offices:

GE Healthcare Bio-Sciences AB
Björkgatan 30 751 84

Uppsala
Sweden

GE Healthcare Europe GmbH
Munzinger Strasse 5 D-79111
Freiburg
Germany

GE Healthcare UK Limited
Amersham Place
Little Chalfont
Buckinghamshire
HP7 9NA
UK

GE Healthcare Bio-Sciences
Corp
800 Centennial Avenue
PO. Box 1327
Piscataway
NJ 08855-1327
USA

GE Healthcare Bio-Sciences KK
Sanken Bldg. 3-25-1
Hyakunincho Shinjuku-ku
Tokyo 169-0073
Japan

GE Healthcare regional office contact numbers:

Asia Pacific
Tel: +85 65 62751830
Fax: +85 65 62751829

Australasia
Tel: + 61 2 8820 8299
Fax: +61 2 8820 8200

Austria
Tel: 01/57606-1613
Fax: 01/57606-1614

Belgium
Tel: 0800 73 890
Fax: 02 416 8206

Canada
Tel: 1 800 463 5800
Fax: 1 800 567 1008

Central, East, & South East Europe
Tel: +43 1 972 720
Fax: +43 1 972 722 750

Denmark
Tel: 45 70 25 24 50
Fax: 45 45 16 2424

Eire
Tel: 1 800 709992
Fax: +44 1494 542010

Finland & Baltics
Tel: +358 9 512 3940
Fax: +358 9 512 39439

France
Tel: 01 69 35 67 00
Fax: 01 69 41 98 77

Germany
Tel: 0800 9080 711
Fax: 0800 9080 712

Greater China
Tel: +852 2100 6300
Fax: +852 2100 6338

Italy
Tel: 02 26001 320
Fax: 02 26001 399

Japan
Tel: +81 3 5331 9336
Fax: +81 3 5331 9370

Korea
Tel: 82 2 6201 3700
Fax: 82 2 6201 3803

Latin America
Tel: +55 11 3933 7300
Fax: + 55 11 3933 7304

Middle East & Africa
Tel: +30 210 96 00 687
Fax: +30 210 96 00 693

Netherlands
Tel: 0800-82 82 82 1
Fax: 0800-82 82 82 4

Norway
Tel: +47 815 65 777
Fax: +47 815 65 666

Portugal
Tel: 21 417 7035
Fax: 21 417 3184

Russia, C.I.S. & N.I.S
Tel: +7 495 956 5177
Fax: +7 495 956 5176

Spain
Tel: 902 11 72 65
Fax: 935 94 49 65

Sweden
Tel: 018 612 1900
Fax: 018 612 1910

Switzerland
Tel: 0848 8028 10
Fax: 0848 8028 11

UK
Tel: 0800 515 313
Fax: 0800 616 927

USA
Tel: +1 800 526 3593
Fax: +1 877 295 8102

<http://www.gehealthcare.com/lifesciences>

GE Healthcare UK Limited

Amersham Place, Little Chalfont, Buckinghamshire, HP7 9NA
UK



imagination at work